NeuWave™

1 System Set-Up

WATCH STEPS 1-5 >

Surgical Procedures:
Step-by-Step Guide

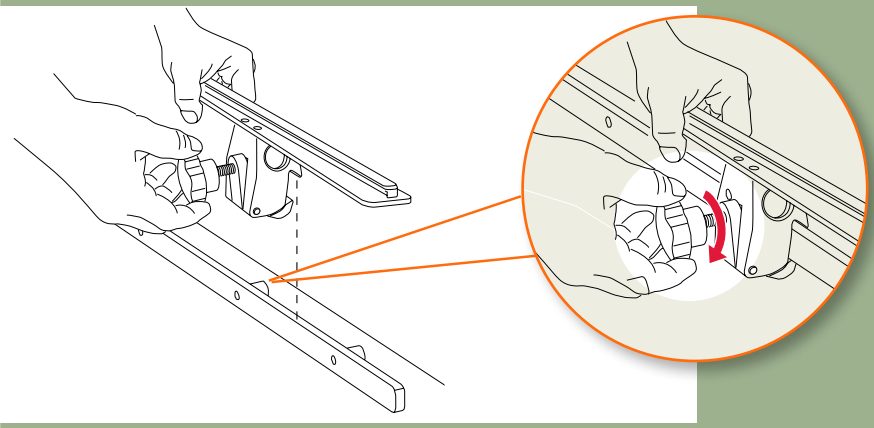

1 Install Bed Rail mount to surgical table rail (optional).

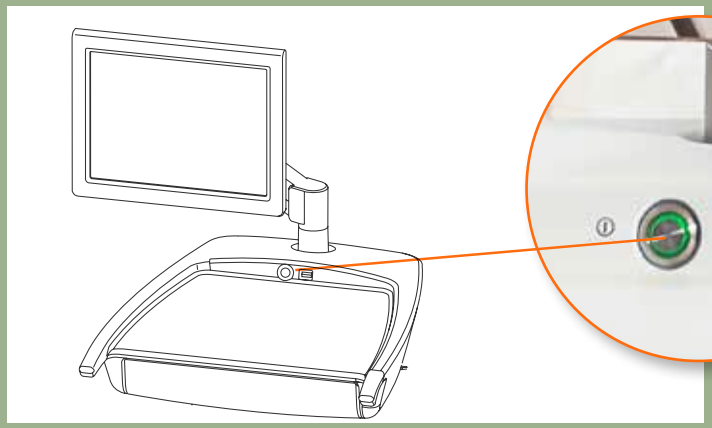

2 Connect system to a hospital-grade AC wall outlet & press ON.

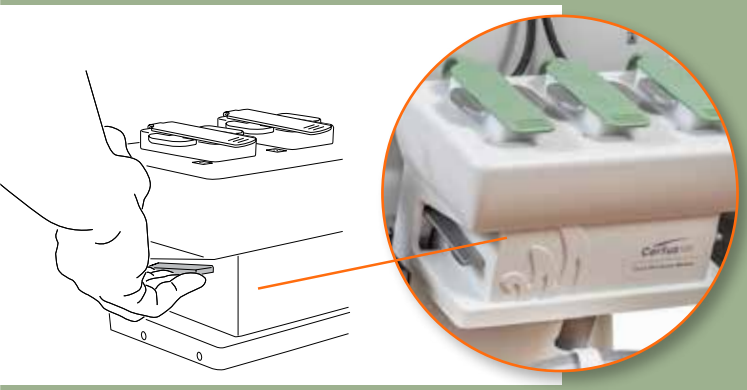

3 Raise & hold both PDM release levers to attach microwave to dovetail rail (optional).

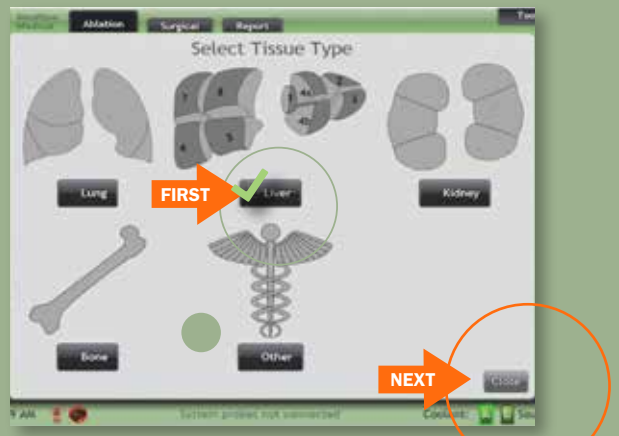

4 Select Tissue Type, then press "Close" on bottom right of screen.

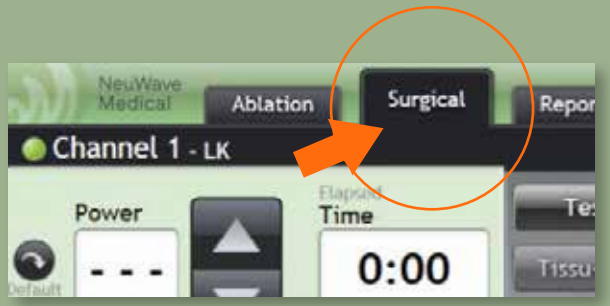

5 Select Surgical Tab to complete set-up.

2 Ablation Procedure

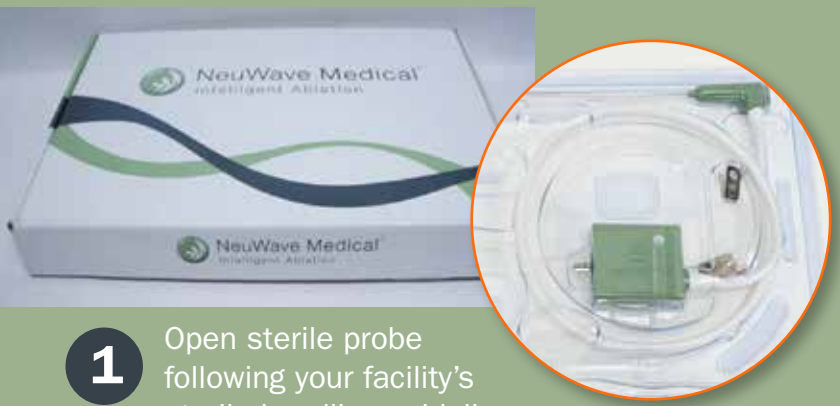

1 Open sterile probe following your facility's sterile handling guidelines.

2 Sterile Technician will hand off probe connector to non-sterile Circulator.

WATCH STEPS 1-6 >

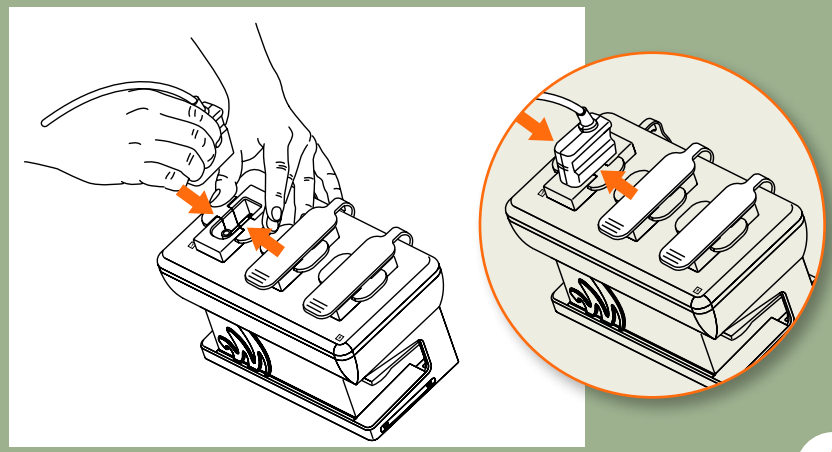

3 Insert probe connector while holding down on silver tab. Press firmly until audible click is heard.

If probe connector doesn't lock, the probe test will fail. This is an easily missed step.

4 To test probe, submerge green tip in a clean container of sterile water.

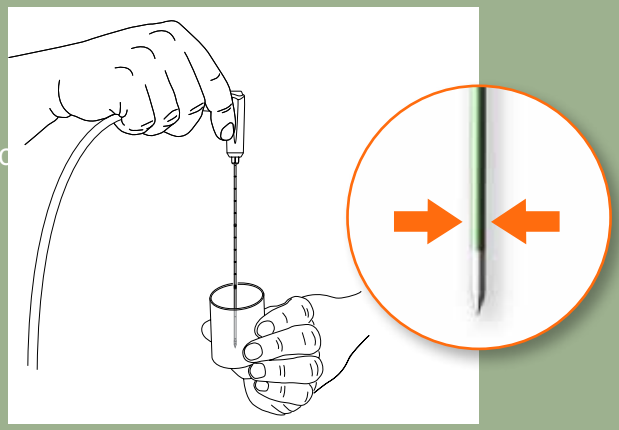

5 For easy step-by-step instructions on how to assemble Surgical Clip: scan QR Code >

6 For both Channels, select “Test” button while watching for bubbles around tip. At end of test, system will ask if bubbles appeared. Select “bubbles” or “no bubbles” icon.

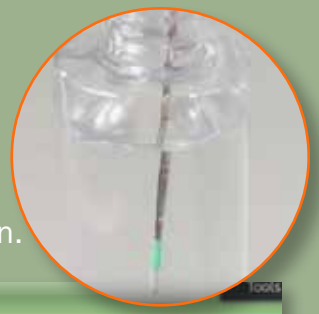

7 For each Channel, set the “Power” (Watts) using the arrows. Power delivery can be set to a maximum of one minute. Note the time set is shown under 0:00.

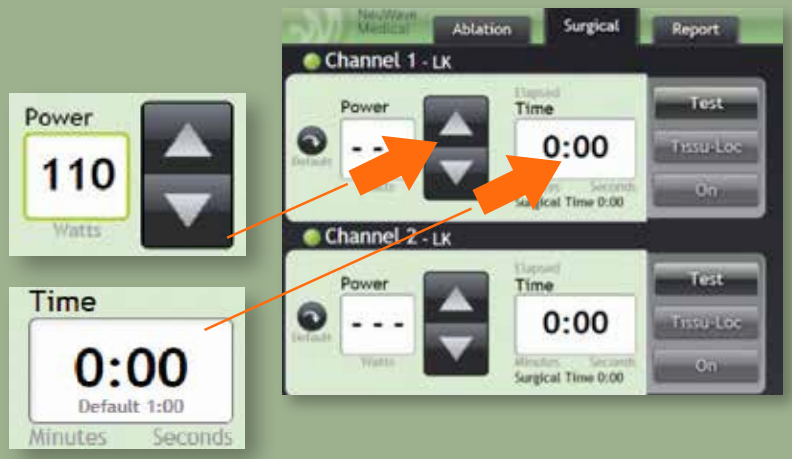

8 When physician is ready to ablate, press “Ablate 1+2” button on bottom to turn on all plugged-in channels. Repeat cycle as many times as needed.

3 Close Procedure

WATCH STEP 1 & 2 >

1 When case has concluded, press “Close Procedure” button then hit “OK”.

2 Press OFF switch. Wait for monitor to turn black before unplugging power cord.

For complete indications, contraindications, warnings, precautions, and adverse reactions, please reference full package insert.

Disclosure

The NeuWave™ Microwave Ablation System and Accessories are indicated for the ablation (coagulation) of soft tissue in percutaneous, open surgical and in conjunction with laparoscopic surgical settings, including the partial or complete ablation of non-resectable liver tumors. The NeuWave™ Microwave Ablation System and Accessories are not indicated for use in cardiac procedures. The system is designed for facility use and should only be used under the orders of a clinician.

NeuWave™

© NeuWave Medical, Inc. 2026. 259583-231005R1